

FLIR E76 14°

P/N: 78511-1101

Copyright

© 2020, FLIR Systems, Inc.

All rights reserved worldwide. Names and marks appearing herein are either registered trademarks or trademarks of FLIR Systems and/or its subsidiaries. All other trademarks, trade names or company names referenced herein are used for identification only and are the property of their respective owners.

Document identity

Publ. No.: 78501-0101 Commit: 71194 Language: Modified: 2020-10-16 Formatted: 2020-10-16

Website

http://www.flir.com

Customer support

http://support.flir.com

Disclaimer

Specifications subject to change without further notice. Camera models and accessories subject to regional market considerations. License procedures may apply. Products described herein may be subject to US Export Regulations. Please refer to exportquestions@flir.com with any questions.



| Imaging and optical data | | | |
|---------------------------------|---|--|--|
| Infrared resolution | 320 × 240 pixels | | |
| UltraMax (super-resolution) | Yes | | |
| NETD | <50 mK @ +30°C (+86°F) | | |
| Field of view | 14° × 10° | | |
| Minimum focus distance | 1.0 m (3.28 ft.) | | |
| Minimum focus distance with MSX | 1.0 m (3.28 ft.) | | |
| Focal length | 29 mm (1.41 in.) | | |
| Spatial resolution (IFOV) | 0.75 mrad/pixel | | |
| Available extra lenses | 42° (AutoCal) 24° (AutoCal) | | |
| Lens identification | Automatic | | |
| f number | 1.5 | | |
| Image frequency | 30 Hz | | |
| Focus | Continuous LDM One-shot LDM One-shot contrast Manual | | |
| Field of view match | Yes | | |
| Digital zoom | 1-4× continuous | | |





| Detector data | | | |
|---|---|--|--|
| Focal plane array/spectral range | Uncooled microbolometer/7.5–14 µm | | |
| Detector pitch | 17 μm | | |
| Image presentation | | | |
| Resolution | 640 × 480 pixels (VGA) | | |
| Surface brightness (cd/m ²) | 400 | | |
| Screen size | 4 in. | | |
| Viewing angle | 80° | | |
| Color depth (bits) | 24 | | |
| Aspect ratio | 4:3 | | |
| Auto-rotation | Yes | | |
| Touchscreen | Optically bonded PCAP | | |
| Display technology | IPS | | |
| Cover glass material | Dragontrail® | | |
| Programmable buttons | 1 | | |
| Viewfinder | No | | |
| Image adjustment | Automatic Automatic maximum Automatic minimum Manual | | |
| Image presentation modes | | | |
| Infrared image | Yes | | |
| Visual image | Yes | | |
| Thermal fusion | No | | |
| MSX | Yes | | |
| Picture in Picture | Resizable and movable | | |
| Gallery | Yes | | |
| Measurement | | | |
| Camera temperature range | -20 to 120°C (-4 to 248°F) 0 to 650°C (32 to 1202°F) Optional 300 to 1000°C (572 to 1832°F) | | |
| Object temperature range and accuracy (for ambient temp. 15 to 35°C (59 to 95°F) | Range -20 to 120°C (-4 to 248°F): -20 to 100°C (-4 to 212°F): ±2°C (±3.6°F) 100 to 120°C (212 to 248°F): ±2% Range 0 to 650°C (32 to 1202°F): 0 to 100°C (32 to 212°F): ±2°C (±3.6°F) 100 to 650°C (212 to 1202°F): ±2% Optional Range 300 to 1000°C (572 to 1832°F): ±2% | | |
| Screening mode | | | |
| Sampling average mode | Recommended temperature range: 30 to 45°C (86 to 113°F) in stable room temperature Accuracy (drift): ±0.3°C (±0.5°F) ¹ | | |

1. No external blackbody needed.





| Inspection mode | | | |
|-------------------------------------|---|--|--|
| FLIR Inspection route | Enabled in the camera | | |
| Measurement analysis | | | |
| Spotmeter | 3 in live mode | | |
| Area | 3 in live mode 3 in live mode | | |
| Automatic hot/cold detection | Auto-maximum/minimum markers within area | | |
| Measurement presets | | | |
| | No measurements Center spot Hot spot Cold spot User preset 1 User preset 2 | | |
| Difference temperature | Yes | | |
| Reference temperature | Yes | | |
| Emissivity correction | Yes: variable from 0.01 to 1.0 or selected from materials list | | |
| Measurement corrections | Yes | | |
| External optics/windows correction | Yes | | |
| Alarm | | | |
| Color alarm (isotherm) | Above Below Interval Condensation (moisture/humidity/dewpoint) Insulation | | |
| Measurement function alarm | Audible/visual alarms (above/below) on any selected measurement function | | |
| Set-up | | | |
| Color palettes | Arctic White hot Black hot Iron Lava Rainbow Rainbow HC | | |
| Setup commands | Local adaptation of units, language, date and time formats | | |
| Languages | 21 | | |
| Service functions | | | |
| Camera software update | Using USB cable or SD card | | |
| Storage of images | | | |
| Storage media | Removable memory; SD card (8 GB) | | |
| Time lapse (periodic image storage) | No | | |
| Remote control operation | Using USB cable or Wi-Fi | | |
| Image file format | Standard JPEG, measurement data included. Infrared-only mode | | |
| Image annotations | | | |
| Voice | 60 seconds built-in microphone and speaker (and via Bluetooth) on still images and video | | |
| Text | Text from predefined list or soft keyboard on touchscreen | | |





| Image annotations | | | |
|--|---|--|--|
| Visual image annotation | Yes | | |
| Image sketch | Yes: on infrared images only | | |
| Sketch | From touchscreen | | |
| METERLINK | Wireless connection (Bluetooth) to: | | |
| | FLIR meters with METERLINK | | |
| Compass | Yes | | |
| Laser distance meter information | Yes | | |
| Area measurement information | No | | |
| GPS | Yes: location data automatically added to every still image and the first frame in video from built-in GPS | | |
| Video recording in camera | | | |
| Radiometric infrared-video recording | RTRR (.csq) | | |
| Non-radiometric infrared-video recording | H.264 to memory card | | |
| Visual video recording | H.264 to memory card | | |
| Video streaming | | | |
| Radiometric infrared-video streaming (compressed) | Over UVC | | |
| Non-radiometric video streaming (compressed: IR, MSX, visual, Picture in Picture) | H.264 (AVC) over RTSP (Wi-Fi) MPEG4 over RTSP (Wi-Fi) MJPEG over UVC and RTSP (Wi-Fi) | | |
| Visual video streaming | Yes | | |
| Digital camera | | | |
| Resolution | 5 MP with LED light | | |
| Focus | Fixed | | |
| Field of view | 53° × 41° | | |
| Video lamp | Built-in LED light | | |
| Laser pointer | | | |
| Laser alignment | Position is automatically displayed on the infrared image | | |
| Laser distance meter | Activated by a dedicated button | | |
| Laser | Class 2, 0.05–40 m (1.6–131 ft.) ±1% of measured distance | | |
| Data communication interfaces | | | |
| Interfaces | USB 2.0, Bluetooth, Wi-Fi, DisplayPort | | |
| METERLiNK/Bluetooth | Communication with headset and external sensors | | |
| Wi-Fi | Peer to peer (ad hoc) or infrastructure (network) | | |
| Audio | Microphone and speaker for voice annotation of images | | |
| USB | USB Type-C: data transfer/video/power | | |
| USB standard | USB 2.0 High Speed | | |
| Video out | DisplayPort | | |
| 1 | | | |



FLIR E76 14°

P/N: 78511-1101 © 2020, FLIR Systems, Inc.

#78501-0101; r. 71194;

| Radio | | | |
|--|--|--|--|
| Operating frequency | Bluetooth + EDR/LE: 2402-2480 MHz | | |
| | WLAN 2.4 GHz: 2412–2462 MHz | | |
| | WLAN 5 GHz: 5150–5350 MHz (DFS: only slave mode) | | |
| | Note that frequency band 5150–5350 MHz is for indoor use only, see national regulations. | | |
| RF output (EIRP) | Bluetooth + EDR/LE: < 10 dBm | | |
| | WLAN: < 17 dBm | | |
| Antenna | Integrated PIFA antenna (gain: maximum 1.4 dBi) | | |
| Power system | | | |
| Battery type | Rechargeable Li-ion battery | | |
| Battery voltage | 3.6 V | | |
| Battery operating time | > 2.5 hours at 25°C (68°F) and typical use | | |
| Charging system | In camera (AC adapter or 12 V from a vehicle) or two-bay charger | | |
| Charging time (using two-bay charger) | 2.5 hours to 90% capacity with charging status indicated by LEDs | | |
| Charging temperature | 0°C to +45°C (+32°F to +113°F), except for the Korean market: +10°C to +45°C (+50°F to +113° F) | | |
| External power operation | AC adapter 90–260 V AC, 50/60 Hz, or 12 V from a vehicle (cable with standard plug—optional) | | |
| Power management | Automatic shut-down and sleep mode | | |
| Environmental data | | | |
| Operating temperature range | -15 to +50°C (5-122°F) | | |
| Storage temperature range | -40 to +70°C (-40 to +158°F) | | |
| Humidity (operating and storage) | IEC 60068-2-30/24 hours/95% relative humidity 25–40°C (77–104°F)/two cycles | | |
| EMC | ETSI EN 301 489-1 (radio) ETSI EN 301 489-17 EN 61000-6-2 (immunity) EN 61000-6-3 (emission) FCC 47 CFR Part 15 Class B (emission) | | |
| Radio spectrum | ETSI EN 300 328 FCC Part 15.249 RSS-247 Issue 2 | | |
| Encapsulation | IP 54 (IEC 60529) | | |
| Shock | 25g (IEC 60068-2-27) | | |
| Vibration | 2g (IEC 60068-2-6) | | |
| Drop | Designed for 2 m (6.6 ft.) | | |
| Safety | EN/UL/CSA/PSE 60950-1 | | |
| Physical data | | | |
| | 1 kg (2.2 lb.) | | |
| Weight (including battery) | 1 Kg (2.2 ID.) | | |
| Weight (including battery) Size (L \times W \times H) | $278.4 \times 116.1 \times 113.1 \text{ mm} (11.0 \times 4.6 \times 4.4 \text{ in.})$ | | |
| | | | |
| Size (L × W × H) | 278.4 × 116.1 × 113.1 mm (11.0 × 4.6 × 4.4 in.) | | |





| Physical data | | | |
|----------------------|---|--|--|
| Housing material | PCABS with TPE, magnesium | | |
| Color | Black | | |
| Warranty and service | | | |
| Warranty | http://www.flir.com/warranty/ | | |
| Shipping information | | | |
| Packaging, type | Cardboard box | | |
| Packaging, contents | Accessory Box I: Power supply for battery charger Power supply, 15 W/3 A Printed documentation SD card (8 GB) USB 2.0 A to USB Type-C cable, 1.0 m USB Type-C to HDMI adapter, standard specification UH311 USB Type-C to USB Type-C cable (USB 2.0 standard), 1.0 m Accessory box II: Accessory box III: Front protection fastener Hand strap bracket, left Screws Torx T10 wrench Carabiner hook Front protection Hand strap Lanyard strap, camera Lens cap strap Wrist strap Battery (2 ea) Battery (2 ea) Battery charger FLIR Thermal Studio Starter Hard transport case Infrared camera with lens Lens cap, front Lens cap, front and rear (only for extra lenses) | | |
| Packaging, weight | 5.8 kg (12.8 lb.) | | |
| Packaging, size | 500 × 190 × 370 mm (19.7 × 7.5 × 14.6 in.) | | |
| EAN-13 | 4743254004597 | | |
| UPC-12 | 845188022594 | | |
| Country of origin | Estonia | | |

Supplies & accessories:

- T300238; Macro lens 2.0x with case
- T131171ACC; Remote operation button
- T300030; Option, No radio
- T911997; Tripod
- T911998; HDMI 2-port video splitter
- T300369; Mounting kit (FLIR T5xx, T8xx, Exx)
- T300344; EST Camera kit (FLIR Exx/T5xx/T8xx)
- T850112; Option, Auto-screening
- T850111; Option, Dual streaming
- T130337ACC; Calibration target
- T199330ACC; Battery
- T199346ACC; Hard transport case for FLIR Exx series




FLIR E76 14°

P/N: 78511-1101

© 2020, FLIR Systems, Inc. #78501-0101; r. 71194;

- T199425ACC; Battery charger
- T199557ACC; Accessory Box II
- T199559; High temperature option, +300 to +1000°C
- T199588; IR lens, f=29 mm (14°) with case
- T199589; IR lens, f=17 mm (24°) with case
- T199590; IR lens, f=10 mm (42°) with case
- T911630ACC; Power supply for camera, 15 W/3 A
- T911631ACC; USB 2.0 A to USB Type-C cable, 0.9 m
- T911633ACC; Power supply for battery charger
- T911689ACC; Pouch for FLIR E-series
- T911705ACC; USB Type-C to USB Type-C cable (USB 2.0 standard), 1.0 m
- T911706ACC; Car adapter 12 V
- T911845ACC; USB Type-C to HDMI and PD adapter
- T911846ACC; USB 2.0 A to USB Type-C with Power supply
- T197771ACC; Bluetooth Headset
- T300342; FLIR Screen EST, Perpetual license
- T300083; FLIR Thermal Studio Pro, Perpetual license
- T300341; FLIR Thermal Studio Standard, 1 Year Subscription
- T300258; FLIR Thermal Studio Standard, Perpetual license
- T198583: FLIR Tools+ (download card incl. license kev)
- T198696; FLIR ResearchIR Max 4 (hardware sec. dev.)
- T199013: FLIR ResearchIR Max 4 (printed license kev)
- T199043: FLIR ResearchIR Max 4 Upgrade (printed license kev)
- 4220499; FLIR Research Studio 1 Year Subscription (online activation)
- 4220500; FLIR Research Studio Perpetual License (online activation)
- 4220646; FLIR Research Studio Perpetual License (USB dongle)
- INST-EW-0140; Extended Warranty 1 Year for E53, E75, E85, E95
- INST-EWGM-0135; Premium Service Package for A35, A65, E53, E75, E85, E95
- INST-GM-0125; General Maintenance Package for A35, A65, Exx, Kxx

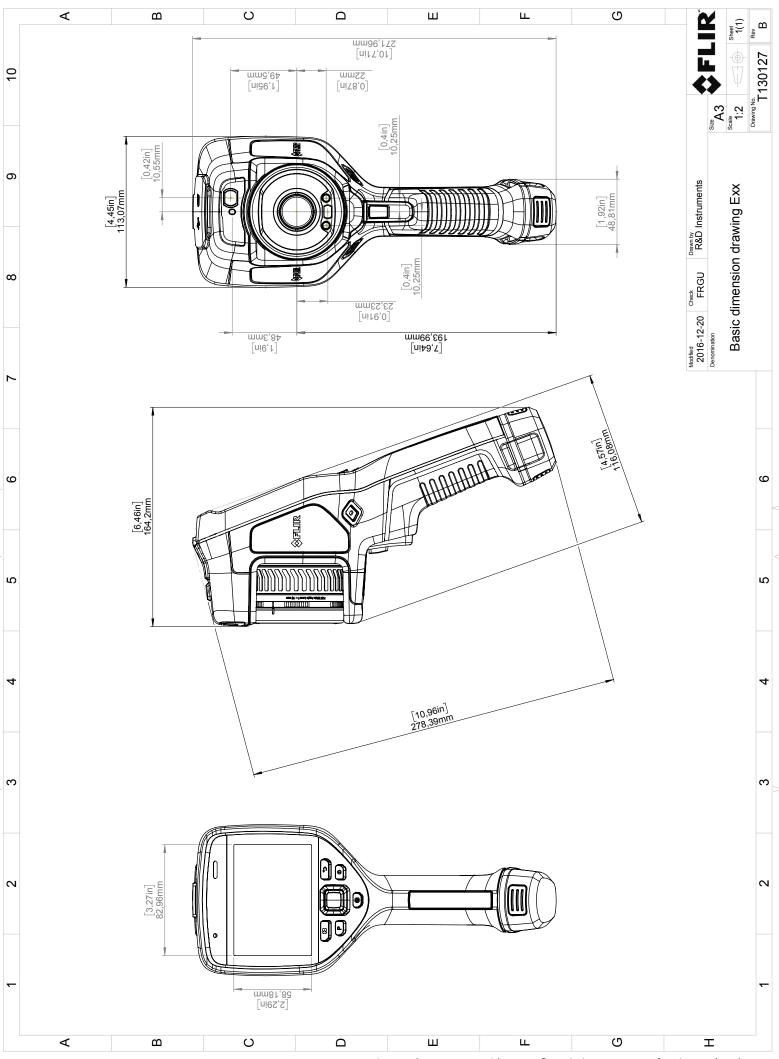

© 2016, FLR Systems, Inc. All rights reserved worldwide. No part of this drawing may be reproduced, stored in a retrieval system, or transmitted in any form, or by any means, electronic, mechanical, photocopying, recording, or otherwise, written permission from FLR Systems, Inc. Specifications subject to change without further notice. Dimensional data is based on nominal values. Products may be subject to regional market considerations. License procedures may apply. Product may be subject to usgoinal market considerations. License procedures may apply.



August 26, 2020 Täby, Sweden

AQ320222

CE Declaration of Conformity – EU Declaration of Conformity

Product: FLIR E53 /E54 /E75 /E76 /E85 /E86 /E95 /E96 -series Name and address of the manufacturer: FLIR Systems AB PO Box 7376 SE-187 15 Täby, Sweden

This declaration of conformity is issued under the sole responsibility of the manufacturer. The object of the declaration: FLIR E53 /E54 /E75 /E76 /E85 /E86 / E95 /E96-series (Product Model Name FLIR-E7850).

The object of the declaration described above is in conformity with the relevant Union harmonisation legislation:

Directives:

| Directive Directive Directive Directive | 2012/19/EU 2014/53/EU 1999/519/EC 2011/65/EU | Radio Equipme | II and electric equipment nt Directive (RED) oposure to electromagnetic fields (SAR) /830/EU | |
|--|---|---|---|--|
| Standards: | | | | |
| Emission: | EN 61000-6-3/ | A1:2011 | Electromagnetic Compability | |
| | | | Generic standards – Emission | |
| Immunity: | EN 61000-6-2: | 2005 | Electromagnetic Compability | |
| | Draft EN 30148 | 89-1:2016 v2.1.0 | Generic standards – Immunity | |
| | EN 301489-17: | 2012 v2.2.1 | | |
| Laser: | EN 60825-1 | | Safety of laser products | |
| Radio: | ETSI EN 300 32 | 28 v1.9.1,v2.1.1 | Harmonized EN covering essential requirements of the R&TTE Directive | |
| | ETSI EN 301 89 | 3 v1.8.1 | Harmonized EN covering essential reqs | |
| SAR: | EN 62209-2 | | Human exposure Wireless | |
| Safety (Battery charger | ·): | | Information technology equipment | |
| | IEC 60950-1:20 | IEC 60950-1:2005+A1 EN 60950- | | |
| | 1:2006+A11:20 | A11:2009+A1:2010+A2:2013+AC:2011+A12:2011 | | |
| RoHS: | EN 50581:2012 | 2 | Technical documentation | |

FLIR Systems AB Quality Assurance

ter Jolon

Lea Dabiri Quality Manager

PO Box 7376, SE-187 15 Täby Sweden [T] +46 8 753 25 00 [F] +46 8 753 23 64 www.flir.com